

09/888,005  
1 of 6


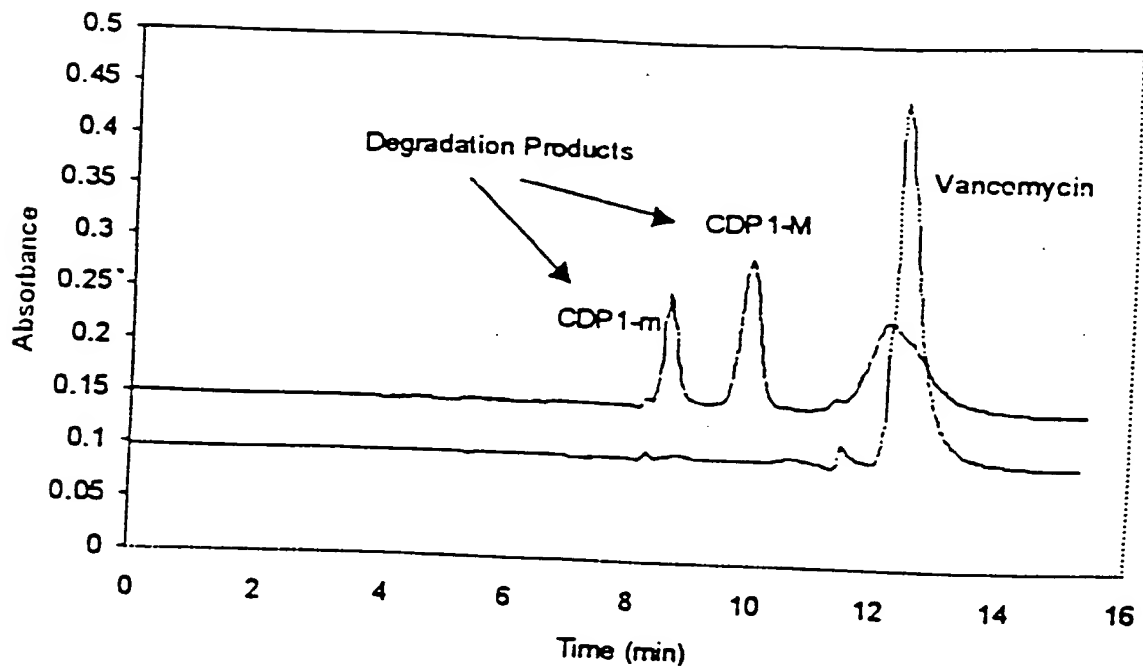


Figure 1.

0988005 062290" 50088860

09/888,005  
2 of 6

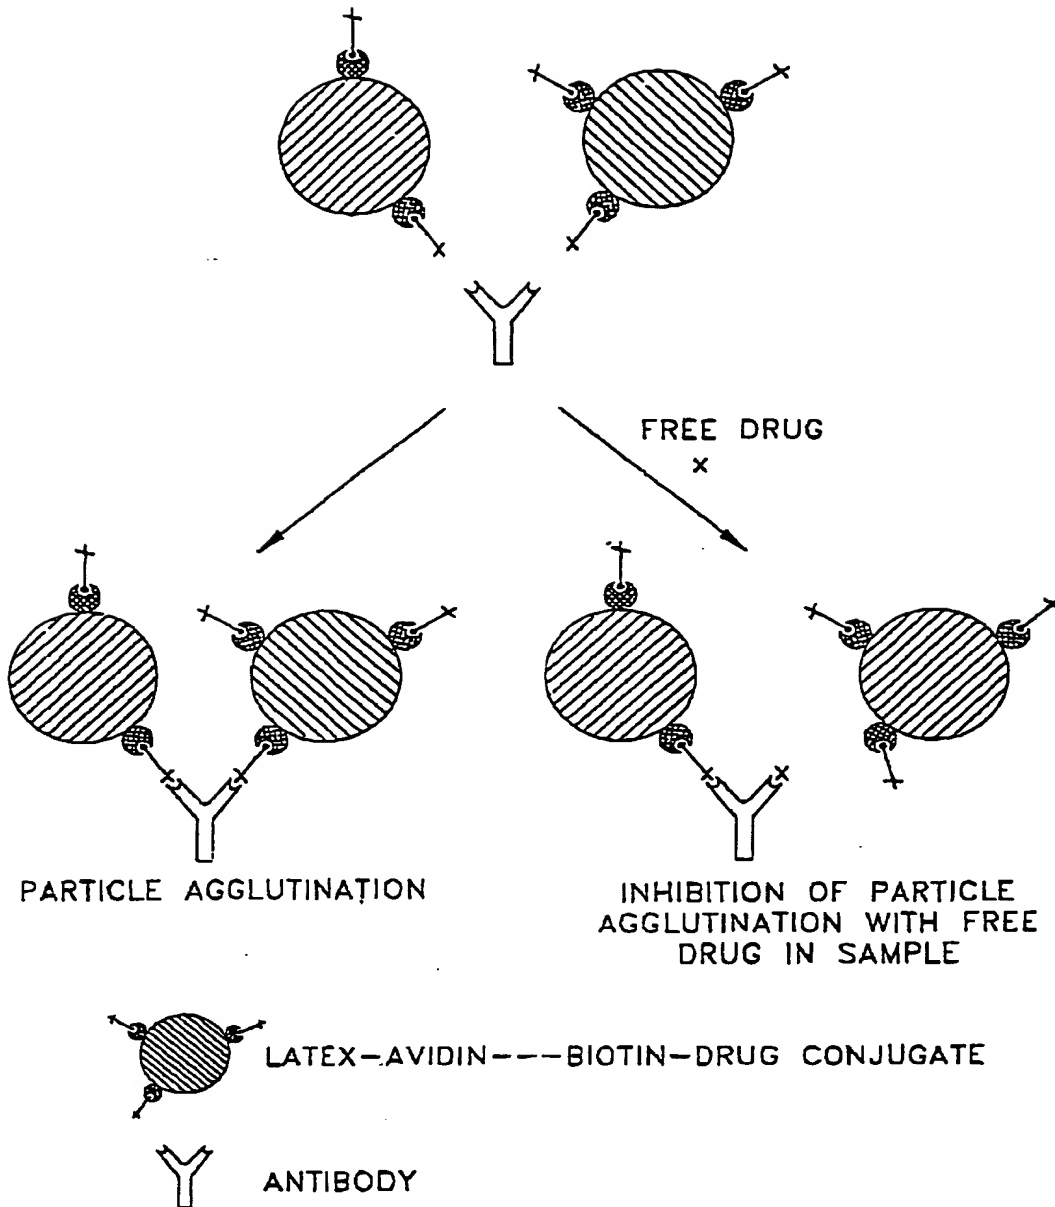

LATEX-BASED BIDENTATE IMMUNOINHIBITION ASSAY -  
2-REAGENT SYSTEM

FIG. 2

09888005-062201

09/888,065  
346

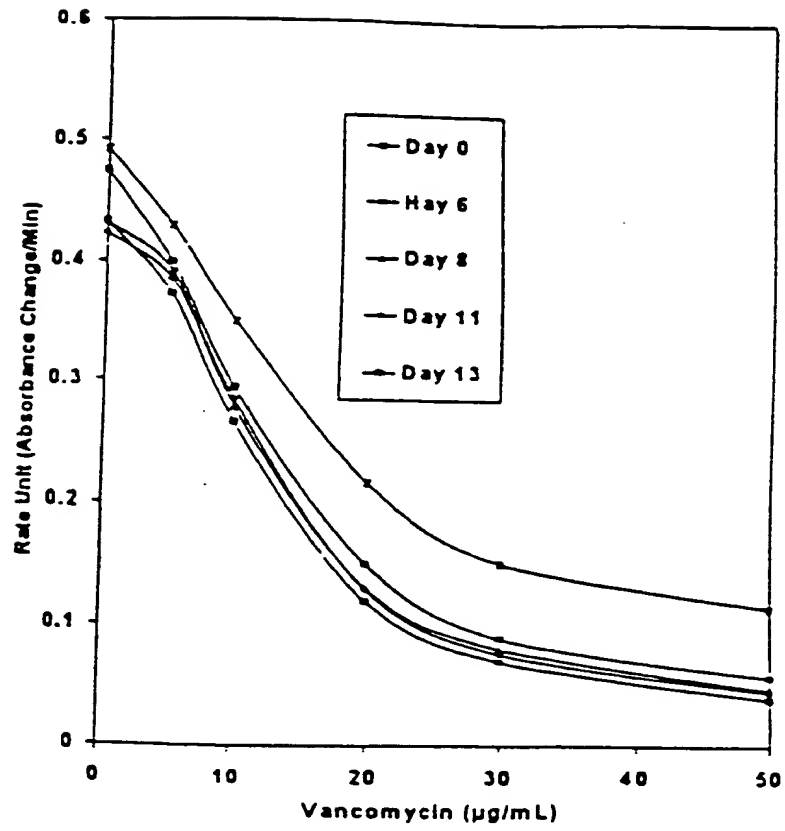


Figure 3

102290" 50088266

09/888,005  
4 of 6

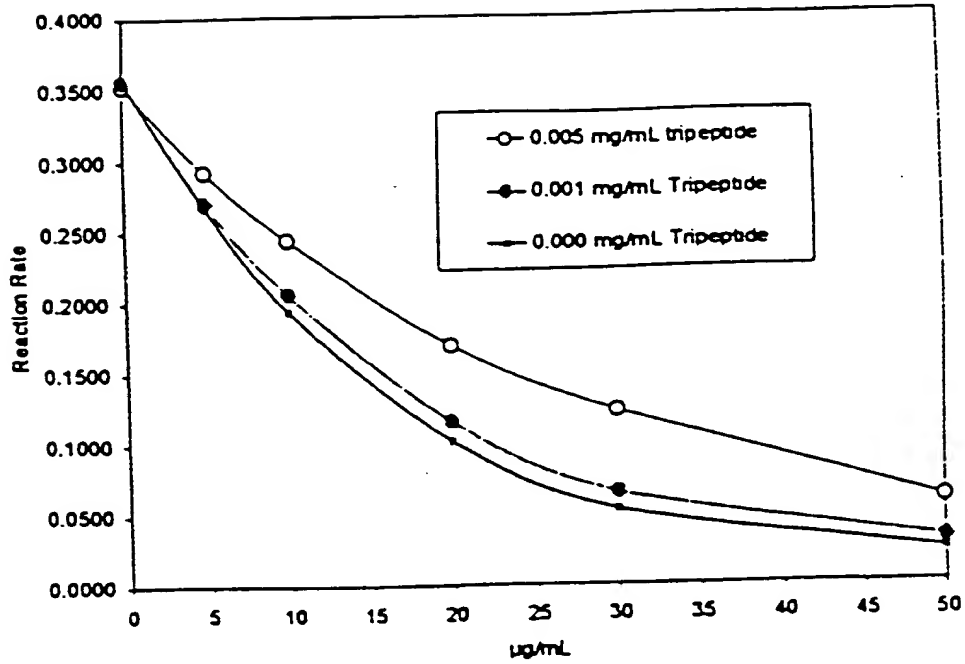


Figure 4

0988005 062201 50088860

09/888,005  
5 y 6

102290" 50088860

CX5 - Synchron (mg/ml)

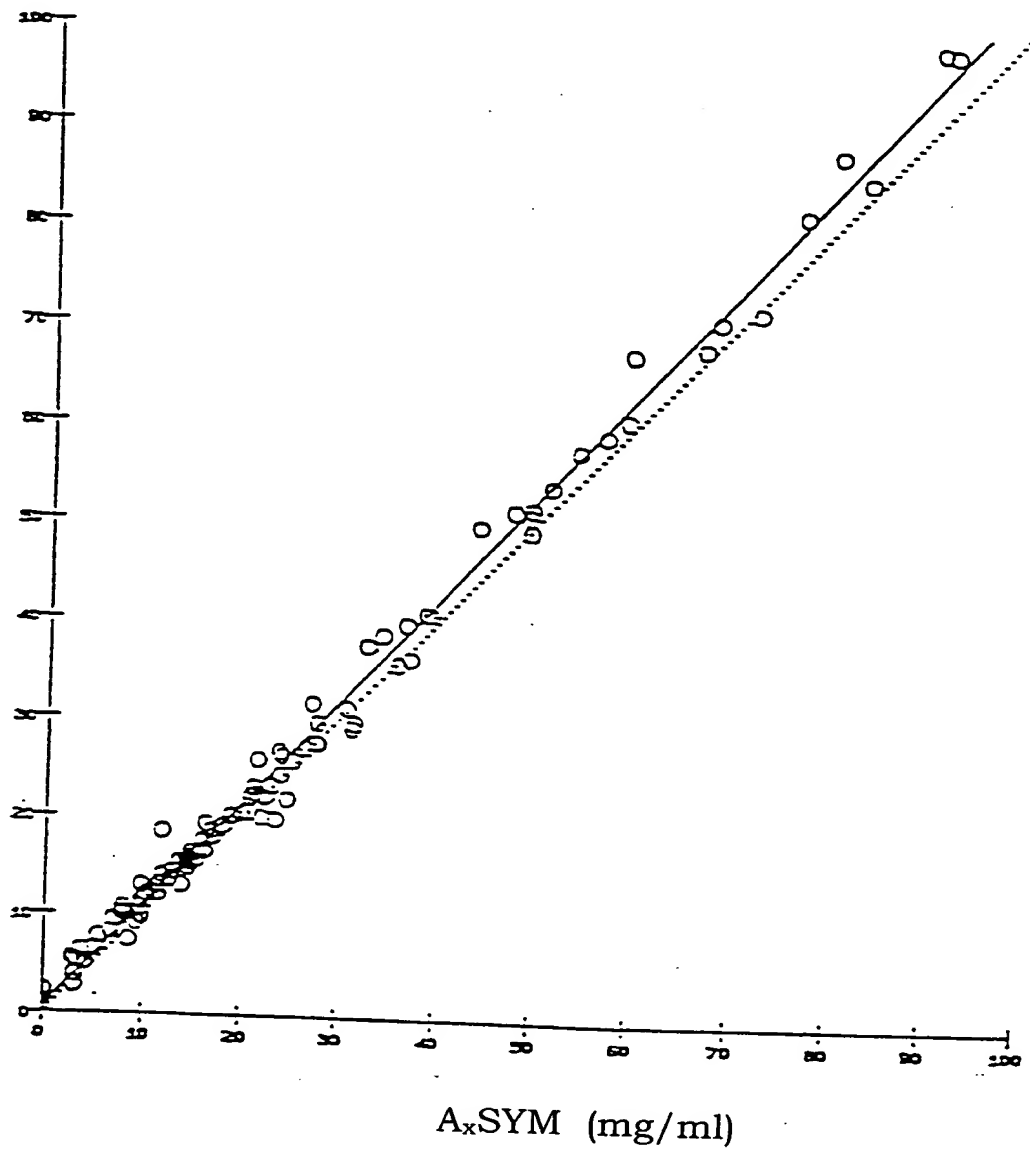


Figure 5

09/888,005  
6 of 6

Fig. 6A

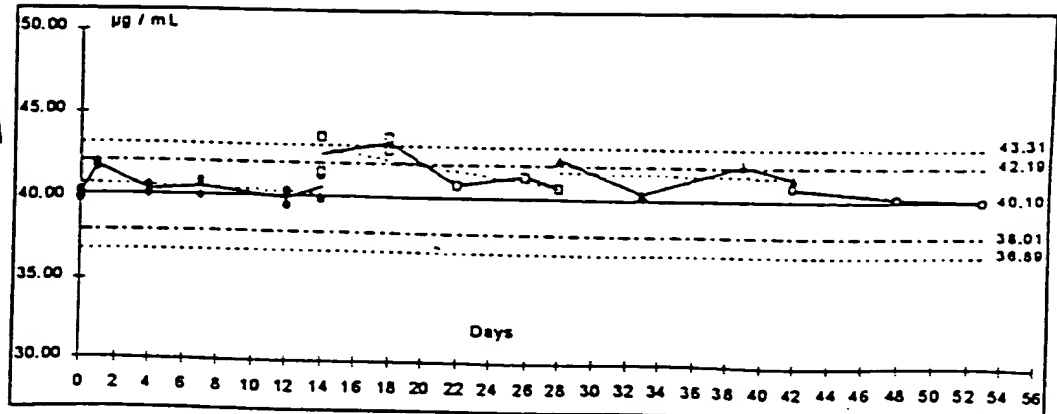


Fig. 6B


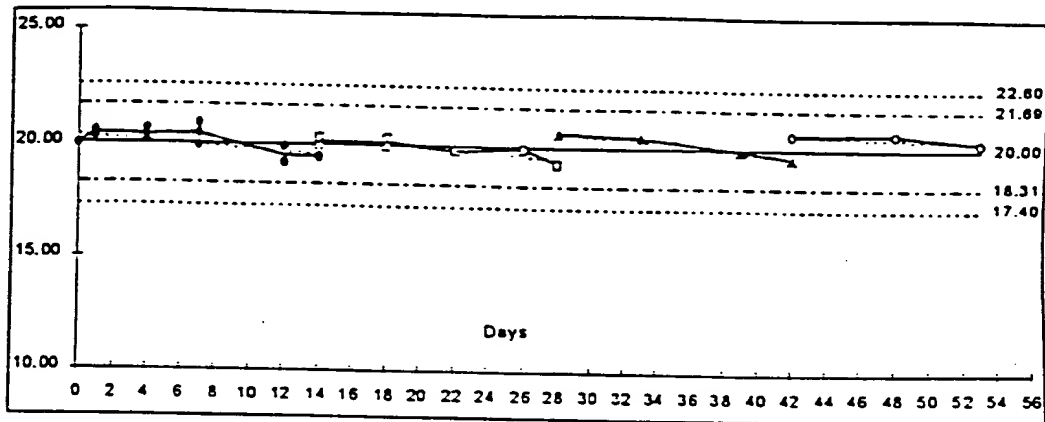


Fig. 6C

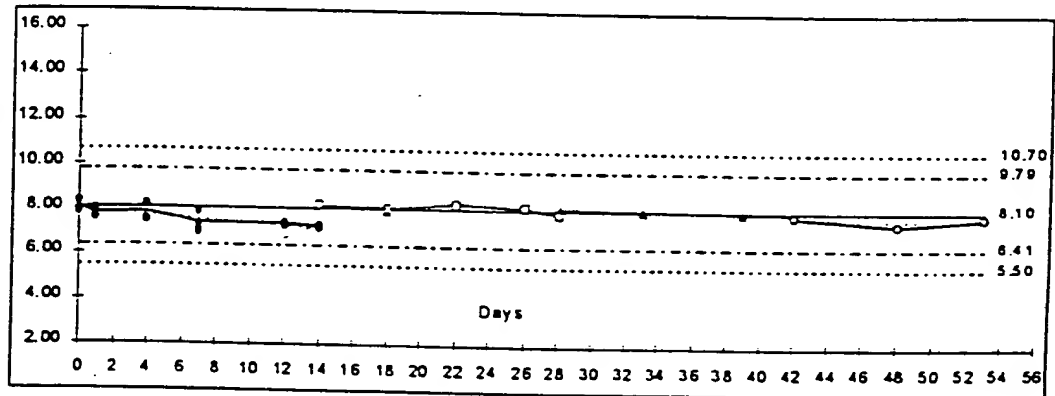

0988005-062201